

Do Placement Of Orthodontic Mini-Implants In Different Locations Improve Skeletal Effects In Herbst Appliance

Kepa Beitia De Busturia^{1*}, Andre Walter Solana² and Andreu Puigdollers Perez³

University Internacional de Catalunya. C/ de Josep Trueta, 08195 Sant Cugat del Vallès, Barcelona. Barcelona, ES 08195

***Corresponding author:**

Kepa Beitia De Busturia,

University Internacional de Catalunya. C/ de Josep Trueta, 08195 Sant Cugat del Vallès, Barcelona. Barcelona, ES 08195.

Tel: 688697074

Received Date: 15 February 2024

Accepted Date: 24 February 2024

Published Date: 29 February 2024

Citation:

Kepa Beitia De Busturia. Do Placement Of Orthodontic Mini-Implants In Different Locations Improve Skeletal Effects In Herbst Appliance. Annals of Clinical and Medical Case Reports 2024.

1. Abstract

1.1. Objective: The aim of this study is to compare dental and skeletal effects in Herbst appliance treatment without anchorage, with interradicular skeletal anchorage and with skeletal anchorage in the external oblique line.

1.2. Design: Non-randomized clinical trial

1.3. Setting: Department of Orthodontics and Dentofacial Orthopedics, Universitat Internacional De Catalunya (UIC), Barcelona, Spain.

1.4. Subjects: Forty eight patients were selected and divided in 3 different anchorage groups.

1.5. Methods: Patients were divided into Control Group (CG), Interradicular Group (IRG) and External Oblique Line Group (EOLG). Measurements were made using lateral craneal X-ray before and after the Herbst appliance use (T1 and T2)

1.6. Results: During the orthopedic treatment, 5 patients were excluded, 4 in the IRG and 1 in EOLG due to loss of implants. Skeletal anchorage has shown less lower incisors inclination in comparison to the control group (CG=8,4°, IRG=2,9°, EOLG=1,7°). WITS values instead were significant in both skeletal groups compared to the control group (EOLG/p=0,001

and IRG/ p=0,001). Regarding ANB values, just CG versus EOLG group comparison was statistically significant (p=0,003).

1.7. Conclusions: The combination of orthodontic mini-implants with the Herbst appliance improved the skeletal response by reducing the excessive lower incisor inclination and improving WITS and ANB values. The mandibular buccal shelf location provided greater OMIs stability and less OMIs failure, that is why it should be selected to avoid implants mobility during the orthopedic treatment.

2. Introduction

Since noncompliance of fixed appliances were introduced in Orthodontics, there has been a major improvement in the treatment of Class II cases. In the last couple of decades, some fixed devices, such as the Herbst appliance, were popularized to advance the mandible in the comprehensive Class II treatment. Herbst appliance causes an advanced mandibular positioning, creating both orthopedic changes in the condyle and fossa displacements. These changes reduce the overjet and achieve a molar and canine class I relationship. These devices, if not stabilized to OMIs (Orthodontic Mini Implants), may present adverse effects such as excessive inclination of the lower incisor and loss of lower molar anchorage. Maximum anchorage with OMIs located in the mandible minimizes or eliminates the mentioned side effects, creating new and more efficient protocols. Therefore, when forces are applied for orthopedic purposes, OMIs provide skeletal anchorage, although they are not always fully stable. Amongst stability factors that play an important key role are implants size and location, secondary stability, root proximity, bone density and cortical bone thickness. For instance, the stability of OMIs placed in the mandible may vary if the implants are located in the anterior or posterior part, due to the specific anatomical characteristics of these regions. Due to these parameters, mandibular OMIs in Herbst appliance could be placed in 2 sites: either interradicularly (IR) (between lower premolars) or in the external oblique line (EOL) also known as mandibular buccal shelf (MBS). This last position provides greater cortical bone thickness and allows bigger OMIs to improve stability. Objectives The objective of this study is to compare dental and skeletal effects in Herbst appliance treatment without anchorage, with interradicular skeletal anchorage and with skeletal anchorage in the external oblique line.

3. Materials and Methods

Forty eight patients participated in this study. Class II skeletal malocclusion were treated with the same Herbst appliance in a period of 18-24 months. Data for the study was collected in Universitat Internacional de Catalunya. The patients were informed through a written

Annals of Clinical and Medical Case Reports

consent, whereby they approved of their willingness to participate in this study. These patients were randomly divided into 2 groups for skeletal anchorage. The Herbst Group (n=19) with only dental anchorage was obtained from previous treatments and was selected as control group (CG); Two groups with skeletal anchorage were studied, one with OMI's located in External Oblique Line of mandible (EOLG) (n=10) and the other with OMI placed Interradically (IRG) (n=14). Patients' age was 12 ± 1.9 in average. The mean treatment time with Herbst appliance was 10 ± 1.7 months. Measurements were made at T1 - Immediately after Herbst appliance and OMI's placement and at T2 - Period of time of 1 month after Herbst appliance removal. The measurements in this study consist in the inclination of the lower incisor related to mandibular plane (incisor mandibular plane angle IMPA, norm $90^\circ \pm 2^\circ$), the sagittal discrepancy between the A-point (deepest point of the concave in the anterior maxilla) and B-point (deepest point of the concave in the anterior mandible) in the cephalometric Steiner values ANB discrepancy (norm $2^\circ \pm 2^\circ$), and the Wits analysis discrepancy (norm 0 ± 1 mm) (drawing perpendiculars from A-point and B-point to the occlusal plane).

The inclination measurements of the OMI's were done from the OMI'S axis line to the mandibular plane line, before and after loading. This measuring methodology was used by several operators in longitudinal clinical studies on orthodontic mini-implants at the anteriorposterior and lateral-medial locations or longitudinal displacement, being a useful accuracy and reliability tool. Both OMI's were measured in this study by two different clinicians (indicated as MT1 and MT2 in table 1 and 2) in order to establish coefficient of correlation. The OMI that was measured and added to the statistic, was the one most visible in the Xray. In this study, inclusion criteria were: patients in age of growth between 10 and 14 years old with a cephalometric Steiner ANB range between $+4^\circ$ and $+7^\circ$. The exclusion criterion in this study was the loss of miniimplants during the orthopedic treatment, extraction cases, breakage of the Herbst appliance more than 2 times in the same patient, previous lower incisor gum recession and patient with poor hygiene and gingivitis. The Herbst appliance (Herbst Developer HD, Tiger Dental, Bregenz, Austria) used for treatment was placed after bracket placement (MBT prescription) approximately 6 - 8 months after starting the orthodontic treatment.

The brackets were placed to level and align the dental arches. Between the 3rd and 5th month of fixed appliance, OMI's were placed bilaterally in the mandible and unloaded for another 2 months to allow secondary stability. OMI's in the interradicular spaces where 1.6 mm diameter x 10 mm length (Jeil Medical corporation, Jet-screw JS, Korea, Seoul), and in the EOLG the OMI's sized 2.0 mm diameter x 14 mm length (Jeil Medical Corporation, Jet-screw- Korea, Seoul). A cephalometric xray (Orthophos SL 3D Sirona, Germany) was done just before the Herbst appliance placement (T1) and after its removal (T2) and dental, skeletal and mini-implants measurements were carried out with the software cephalometric analysis Nemoceph (Nemotech Biotech Dental Company, Madrid, Spain). Activations of the Herbst appliance in steps of 2-3 mm were done every 3 months gradually.

3.1. OMI's Placement Protocol:


OMI's placement were performed under local anesthesia. A straight screwdriver did the insertion vertically in the IRG manually and a contraangle piece was used in the EOLG. After placement, the mini implants were untouched and unloaded during a healing period of 4-8 weeks in order to establish secondary stability. OMI's loading was made with a 0,12 metal ligature in the molar bands (EOLG) and in the lower canines brackets (IRG). (Figure 1-4).



Figure 1



Figure 2

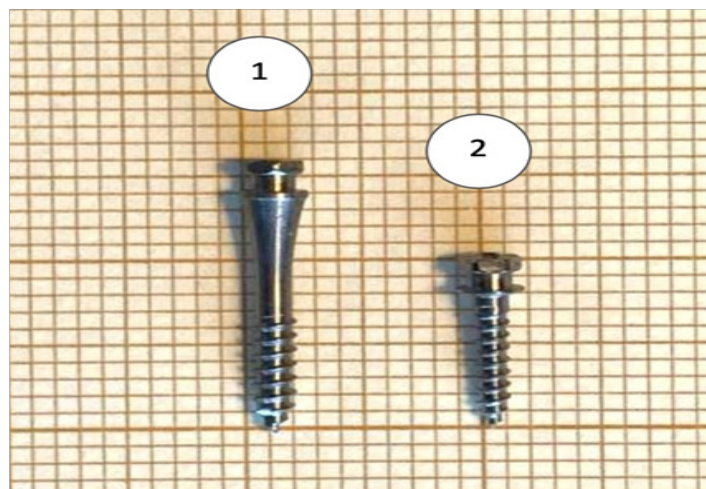

Annals of Clinical and Medical Case Reports

Figure 3

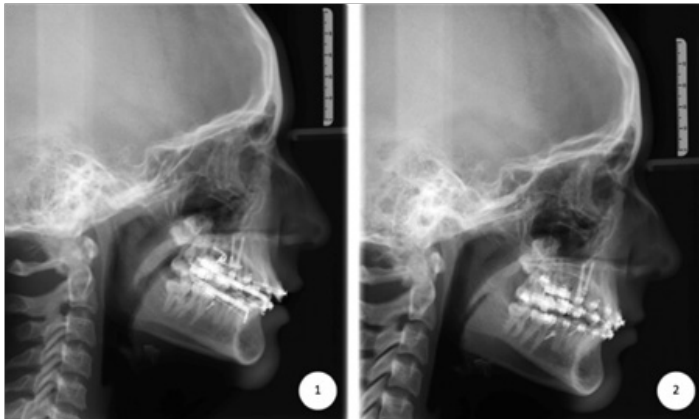


Figure 4

3.2. Statistical Analysis:

Five patients were excluded in this study, 4 in the IRG and 1 in EOLG due to loss of implants. Descriptive analysis was conducted. Categorical variables were described with frequencies and percentages, while quantitative variables were described with mean, standard deviation, median, quartiles, minimum and maximum. To assess the statistical differences between the control groups, IRG and OELG a Kruskal-Wallis test were performed, and to evaluate pairwise differences between groups,

Mann-Whitney U test were used. In all analysis p-values less than 0.05 were considered statistically significant. Analysis conducted with SPSS 25.0 (IBM Corp.).

4. Results

During the orthopedic treatment, 5 patients were excluded, 4 in the IRG and 1 in EOLG due to loss of implants. The patients treated with skeletal anchorage (IR and EOL groups) improved skeletally and obtained a dental correction into a class I. Skeletal anchorage has shown less lower incisors inclination in comparison to the control group (Table 1). The increase inclination of the lower incisor was present in all 3 groups after the treatment (CG=8,4°, IRG=2,9°, EOLG=1,7°). The inclination of the lower incisors was statistically significant between control group and skeletal anchorage groups (p=0.001). Although there were not statistically significant differences between both skeletal anchorage groups (IRG vs EOLG) (p=0,341). The skeletal values of ANB and WITS treated with skeletal anchorage were better in comparison to the control group (Table 2). Regarding ANB values, just CG versus EOLG group comparison was statistically significant (p=0,003). WITS values instead were significant in both skeletal groups compared to the control group (EOLG/p=0,001 and IRG/ p=0,001) (table 2). WITS and ANB improved in the CG 1,7° and 1,8° respectively, -3° and -2,4° respectively in the IRG and lastly, -3,3° and -2,9° respectively in the EOLG (table 1).

Table 1:

			T1 I	T2	Dif	T1	T2	Dif	T1	T2	Dif	T1	T2	Dif	T1	T2	Dif
			MPA	IMPA	IMPA	ANB	ANB	ANB	WITS	WITS	WITS	MT1	MT1	MT1	MT2	MT2	MT2
CG	N	Vaield	19	19	19	19	19	19	19	19	19	0	0	0	0	0	0
		Miss- ing	0	0	0	0	0	0	0	0	0	0	10	10	10	10	10
	Mean	96,42	104,8	8,42	5,21	3,42	1,79	3,5	1,83	1,67							
	St d . Devi- ation	7,676	7,32	4,234	1,389	1,216	0,918	1,901	1,538	1,168							
	Mini- mum	82	95	3	3	1	3	1	2	4							
Maxi- unm		110	118	21	8	5	0	7	4	0							
IRG	N	Vaield	14	14	14	14	14	14	14	14	14	14	14	14	14	14	14
		Miss- ing	0	0	0	0	0	0	0	0	0	0	0	0	0	0	0
	Mean	101,1	104,1	2,93	5,21	2,82	2,39	3,39	0,37	3,02	101,6	104,1	2,57	100,05	102,93	2,43	
	St d . Devi- ation	5,231	5,210	3,626	0,893	1,436	1,112	2,138	1,999	0,95	10,53	11,78	2,875	8,253	7,395	3,251	
	Mini- mum		91	93	3	4	0	5	1	3	4	83	81	3	90	93	3

Annals of Clinical and Medical Case Reports

	Maxi- unm		109	112	9	7	5	1	6	3	2	118	118	6	115	118	7
EO LG	N	Vaild	10	10	10	10	10	10	10	10	10	10	10	10	10	10	10
		Miss- ing	0	0	0	0	0	0	0	0	0	0	0	0	0	0	0
	Mean		103,8	105,5	1,7	5,6	2,7	2,9	4,2	0,95	3,25	101,9	102,1	0,2	100,6	100,8	0,2
	St d . Devi- ation		8,27	7,427	2,541	0,966	0,949	0,568	1,317	1,189	0,825	8,66	9,183	2,573	7,677	8,377	1,687
	Mini- mum		86	89	3	4	1	4	2	2	5	92	94	3	93	92	2
	Maxi- unm		112	115	6	7	4	2	6	2	2	119	122	3	117	120	3

The inclination of OMI regarding the mandibular plane (Go-Gn) showed a better stability in the EOLG rather than in the IRG. MT1 and MT2 measurement showed OMI mesial inclination of 2,57° and 2,43° respectively in the IR group. For EOL group, MT1 and MT2 measurements were an increased inclination of 0,2° in both measurements (table 1). Difference between both groups IRG and EOLG was indeed less than 2,5° (p=0,022 in MT1 and p=0,064 in MT2). The two groups with the skeletal anchorage, IRG and EOLG, did not show any significant differences in the inclination of the lower incisors, the ANB nor in the WITS values (p=0,341; p=0,172; p=0,709 respectively). In this study 5 OMI lost stability during treatment and were taken out of the study. OMI failed more frequently in the IRG than in the EOLG. The OMI failure relation between the IRG and the EOLG was 4:1.

5. Discussion

Herbst has been demonstrated to be an effective tool to correct skeletal Class II malocclusions. It has a dental effect that reduces the overjet by means of proinclination of the lower incisors. The combination of skeletal effect and proinclination of the lower incisor, contributes in the correction of the Class II malocclusion, and establishes a Class I dental relationship. Other techniques have tried to control the inclination of the lower incisor such as torque control information in the stainless steel arches or brackets slot information. Though, in most occasions this inclination was already increased before treatment because of mandible retrusion with compensatory proinclination. For this reason, further proinclination should be avoided during the correction of the sagittal discrepancy, indicating that skeletal anchorage is a useful tool. The Herbst appliance used in this study had the disadvantage of moving the teeth (more easily) buccally due to the vestibular braces position before the desirable orthopedic effect. Therefore, it adversely favors a greater proinclination of the lower incisor when compared to other Herbst that work without braces. It is for this reason, that the use of miniimplants is highly recommended, especially in orthopedic class II appliances designs that works in combination with braces. During the design of the study, in the most severe cases the patient's parents were duly informed to perform an orthognathic

surgery treatment with mandibular advancement. Those patients who refused the surgical alternative were assigned to the randomized study. The selection of the patients to use Herbst appliance in combination with OMI placement was recommended in those patients with inclination of the lower incisors to the mandible plane greater than 100° to avoid further incisor proinclination during the orthopedic treatment in the sagittal discrepancy. A randomized method to assign the control group in patients with very proinclined lower incisors was considered inappropriate and unethical, and therefore the randomization within these patients was only assigned to the conventional device-anchoring mode, interradericular vs. external oblique line. This was done to avoid the unnecessary risk of potential gingival injuries. The Herbst appliance used and the bracket system prescription were the same for each patient in order to control the variables of the study. With the aid of interproximal enamel reduction techniques used during the alignment and leveling phase, no additional inclination of the lower incisor further than 2mm occurred. Exceeding this value meant the exclusion of the study.

Wits analysis was used to assess the severity of the Class II. The values may vary considerably during the correction of the lower arch Curve of Spee and the position of the lower incisor. To reduce the bias of the methodology, the measurement in the cephalometric x-ray was carried out after 6-8 months of the brackets placement with its 0,019x 0,025" stainless steel arch wires in place, once the leveling, alignment and crowding was duly corrected. At this stage, the placement of the Herbst appliance produced few arch wire deformations during orthopaedic mandibular advancement. For similar reasons, the Steiner ANB measurement was performed at the same time as the Wits measurement, since it is known that point A can undergo modifications during correction of the upper incisor inclination, especially in retruded and retroclined upper incisors. Although small degrees differences (between 1-3°) in the measurements before and after the treatment were found, the landmark identification of A and B points in cephalometric Steiner analysis has been proven as a safe, standardized and reliable method of measurement and it demonstrates a more favorable response of the orthopedic treatment with OMI in this study, specifically in the EOLG group (p=0,003). And even if IRG was

Annals of Clinical and Medical Case Reports

not statistically significant, ANB improved $-2,4^{\circ}$ (IRG $p = 0.24$) (table 2). The study demonstrated the efficiency of the skeletal anchorage to prevent the lower incisor from further proinclination (Table 2, $p = 0.001$). It is known that OMI's placed in bone might move when they are loaded under constant forces around 400g, especially those with small diameters and lengths. Cortical bone thickness is also a big factor in this stability loss. Which is why this study was divided in 2 groups of skeletal anchorage. Less interradicular cortical thickness ($<1\text{mm}$) compared to the external oblique line (2-3mm), suggests greater risk of mini-implants failure, as seen in the IRG (4:1). Although these 4 patients were excluded from the study, the anchorage loss in the IRG compared with the EOLG would produce surely statistically more significant skeletal changes, not seen in this study (Table 2, $p = 0.172$ for the ANB analysis, $p = 0.709$ for the Wits analysis). The skeletal effect of the Herbst appliance in combination with OMI's anchorage evaluated in this study coincides with other studies' results. The benefits in Wits skeletal response ($p = 0.001$ in IRG, $p = 0.001$ in EOLG), ranged from $-3,02\text{mm}$ to $-3,25\text{mm}$ (Table 1). A direct orthopaedic load on the mini-implants with the Herbst appliance was not recommended because of the increasing risk of implant failure so an indirect anchoring with a small ligature was used. Lower incisor proinclination as a side effect could not be completely avoided in all samples. Small implants movement during loading or an insufficient wire tightness or tension in the molar bands during the strong orthopaedic forces could have affected the wire ligature or created deformations. The anchorage efficiency between the EOLG and the IRG did show statistically significant differences in

the MT1 measurements ($p = 0,022$) and almost statistically significant differences in the MT2 measurements ($p = 0,64$). Yet, the lower success rate of the OMI's in the IRG suggested that the small OMI's diameter in the interradicular spaces were not as effective for orthopedic forces of 400g, especially in areas with root proximity, where implant mobility could occur. A cephalometric X-ray was taken just before and after the treatment. They were used to measure skeletal structures as Wits, Steiner ANB analysis, OMI's and dental measurements. Comparison of measurements in cephalometric X-rays is described in the scientific literature as a reliable, accurate and safe method, as long as the same X-ray machine is used. Although the landmark identification can lead to errors, measurements were carried out twice by two experienced operators. The OMI's inclination to the mandibular plane was very similar to the method of measuring the inclination of the lower incisor to the mandibular plane. This was possible because the OMI's insertion was carried out in a vertical and apical inclination, facilitating the visualization of its axially and therefore allowing the standardized method of measurements. The inclination of the implants related to the mandible plane revealed that the mini-implants were not stable during the orthopedic loading in the IRG. All treated patients in the 3 groups at the end of the orthopedic treatment reached a molar and canine class I occlusion, confirming the findings of the effectiveness of the Herbst appliance in normalizing the skeletal parameters. When using implants as skeletal anchorage the reduction of the dentoalveolar compensations can improve the skeletal response (Table 1 and 2).

		T1 IMPA	T2 IMPA	Dif IMPA	T1 ANB	T2 ANB	Dif ANB	T1 WITS	T2 ITS	Dif WITS	T1 MT1	T2 MT1	Dif MT1	T1 MT2	T2 MT2	Dif MT2
K-W test		0,024	0,742	0,001	0,596	0,2	0,011	0,561	0,088	0,001	0,906	0,464	0,021	0,68	0,394	0,059
M-W Test	CG vs. IRG	0,05	0,843	0,001	0,9	0,24	0,152	0,957	0,05	0,001						
	CG vs. EOLG	0,16	0,636	0,001	0,403	0,094	0,003	0,308	0,115	0,001						
	IRG vs. EOLG	0,259	0,403	0,341	0,371	0,886	0,172	0,403	0,752	0,709	0,931	0,472	0,022	0,709	0,403	0,064

Therefore, the reduction of the lower incisor inclination during the activations of the Herbst appliance, allows further activations to adequate temporomandibular joint and neuromuscular adaptations in a more anterior mandible position to enhance favorable bone remodeling. The results of the study showed benefits of the OMI's in the skeletal response. Nevertheless, results should be interpreted with caution because there is no statistical difference between these two study groups (EOLG and IRG). And even though no clear differences amongst the IRG and the EOLG were found, with 5 patients excluded from the study, there is a clear tendency towards external oblique line location as a better OMI's location (table 1). Further studies in the OMI's success rate with greater sample size must be carried out in the future to corroborate the ideal OMI's position in combination with the Herbst appliance for the effectiveness of the orthopedic response.

6. Conclusion

The combination of orthodontic mini-implants with the Herbst appliance improved the skeletal response by reducing the excessive lower incisor inclination and improving WITS and ANB values. The mandibular buccal shelf location provided greater OMI's stability and less OMI's failure, that is why it should be selected to avoid implants mobility during the orthopedic treatment.

References

1. AlmeidaMR."Biomechanics of extra-alveolar mini-implants." *Dental-Press Journal of Orthodontics*. 2019;24(4):93-109.
2. Baumgaertel Sand HansMG."Buccal cortical bone thickness for mini-implant placement." *American Journal of Orthodontics and Dental Facial Orthopedics*. 2009.
3. Baysal A and Uysal T. "Dentoskeletal effects of Twin Block and Herbst appliances in patients with Class II division I mandibular retrognathia."

Annals of Clinical and Medical Case Reports

- European Journal of Orthodontics. 2014; 36(2):164-172.
4. Bock N, Ruehl J and Ruf S. "Orthodontic Class II: 1 treatment - efficiency and outcome quality of Herbst-multibracket appliance therapy." *Clinical Oral Investigations*. 2018.
 5. Broch J, Slagsvold O and Røsler M. "Error in landmark identification in lateral radiographic headplates." *European Journal of Orthodontics*. 1981.
 6. Chen YJ, Chang HH, Huang CY, Hung HC, Lai EHH, and Yao CCJ. "A retrospective analysis of the failure rate of three different orthodontic skeletal anchorage systems." *Clinical Oral Implants Research*. 2007.
 7. Chen YJ, Chang HH, Huang CY, Hung HC, Lai EHH and Yao CCJ. "A retrospective analysis of the failure rate of three different orthodontic skeletal anchorage systems." *Clinical Oral Implants Research*. 2007; 18(6):768-775.
 8. Costa A, Raffaini M and Melsen B. "Mini screws as orthodontic anchorage: a preliminary report." *International Journal of Adult Orthodontics and Orthognathic Surgery*. 1998; 13(3):201-209.
 9. Dias LCS, da Costa Ferreira YB, de Jesus Tavares RR, Pinzan-Vercelino CRM and de Araújo Gurgel J. "Reliability and accuracy of radiographic analysis method for posterior maxillary mini-implant location." *Journal of Applied Oral Science*. 2012.
 10. Grogger P, Sacher C, Weber S, Millesi G and Seemann R. "Identification of 'Point A' as the prevalent source of error in cephalometric analysis of lateral radiographs." *International Journal of Oral and Maxillofacial Surgery*. 2018.
 11. Guimarães CH, Henriques JFC, Janson G, De Almeida MR, Araki J, Cançado RH, et al. "Prospective study of dentoskeletal changes in Class II division malocclusion treatment with twin force bite corrector." *Angle Orthodontist*. 2013.
 12. Hiasa K, Abe Y, Okazaki Y, Nogami K, Mizumachi W and Akagawa Y. "Preoperative Computed Tomography-Derived Bone Densities in Hounsfield Units at Implant Sites Acquired Primary Stability." *ISRN Dentistry*. 2011.
 13. Hourfar J, Bister D, Kanavakis G, Lisson JA and Ludwig B. "Influence of interradicular and palatal placement of orthodontic mini-implants on the success (survival) rate." *Head & Face Medicine*. 2017.
 14. Kuroda S, Yamada K, Deguchi T, Hashimoto T, Kyung HM and Yamamoto TT. "Root proximity is a major factor for screw failure in orthodontic anchorage." *American Journal of Orthodontics and Dentofacial Orthopedics*. 2007.
 15. Liou EJW, Pai BCJ and Lin JCY. "Do miniscrews remain stationary under orthodontic forces?" *American Journal of Orthodontics and Dentofacial Orthopedics*. 2004.
 16. Luzi C, Luzi V and Melsen B. "Mini-implants and the efficiency of Herbst treatment: A preliminary study." *Progress in Orthodontics*. 2013.
 17. Luzi C, Verna C and Melsen B. "Guidelines for success in placement of orthodontic mini-implants." *Journal of Clinical Orthodontics*. 2009.
 18. Marcé-Nogué J, Walter A, Gil L and Puigdollers A. "Finite Element Comparison of 10 Orthodontic Miniscrews with Different Cortical Bone Parameters." *International Journal of Oral and Maxillofacial Implants*. 2013.
 19. McClure SR, Sadowsky PL, Ferreira A and Jacobson A. "Reliability of digital versus conventional cephalometric radiology: A comparative evaluation of landmark identification error." *Seminars in Orthodontics*. 2005.
 20. Mosleh MAA, Baba MS, Malek Sand Almaktari RA. "Ceph-X: Development and evaluation of 2D cephalometric system." *BMC Bioinformatics*. 2016.
 21. NCT02411812. "Effects of the Herbst Appliance With Skeletal and Dental Anchorage in Lower Incisors in Class II Malocclusion." *ClinicalTrials.gov*. Retrieved from <https://clinicaltrials.gov/show/NCT02411812>. 2015.
 22. Nienkemper M, Handschel J and Drescher D. "Systematic review of mini-implant displacement under orthodontic loading." *International Journal of Oral Sciences*. 2014; 6(1):1-6.
 23. Nienkemper M, Wilmes B, Renger S, Mazaud-Schmelter M and Drescher D. "Improvement of mini-implant stability in orthodontics." *Orthodontie Française*. 2012; 83(3):201-207.
 24. Pancherz H and Sack B. "A critical analysis of the SNA, SNB and ANB angles in assessing orthodontic treatments." *Fortschritte der Kieferorthopädie*. 1990.
 25. Ruf S and Pancherz H. "Temporomandibular joint growth adaptation in Herbst treatment: A prospective magnetic resonance imaging and cephalometric roentgenographic study." *European Journal of Orthodontics*. 1998.
 26. Ruf S and Pancherz H. "Temporomandibular joint remodeling in adolescents and young adults during Herbst treatment: A prospective longitudinal magnetic resonance imaging and cephalometric radiographic investigation." *American Journal of Orthodontics and Dentofacial Orthopedics*. 1999.
 27. Ruf S and Pancherz H. "Herbst/multibracket appliance treatment of Class II division I malocclusions in early and late adulthood. A prospective cephalometric study of consecutively treated subjects." *European Journal of Orthodontics*. 2006; 28(4): 352-360.
 28. Ruf S, Hönemann S and Pancherz H. "Does orthodontic proclination of lower incisors in children and adolescents cause gingival recession?" *American Journal of Orthodontics and Dentofacial Orthopedics*. 1998.
 29. Samrit V, Kharbanda OP, Duggal R, Seith A and Malhotra V. "Bone density and miniscrew stability in orthodontic patients." *Australian Orthodontic Journal*. 2012.
 30. Wang Z, Zhao Z, Xue J, Song J, Deng F and Yang P. "Pull-out strength of miniscrews placed in anterior mandibles of adult and adolescent dogs: A micro-computed tomographic analysis." *American Journal of Orthodontics and Dentofacial Orthopedics*. 2010.